


Analyst

www.rsc.org/analyst

Volume 137 | Number 15 | 7 August 2012 | Pages 3393–3584

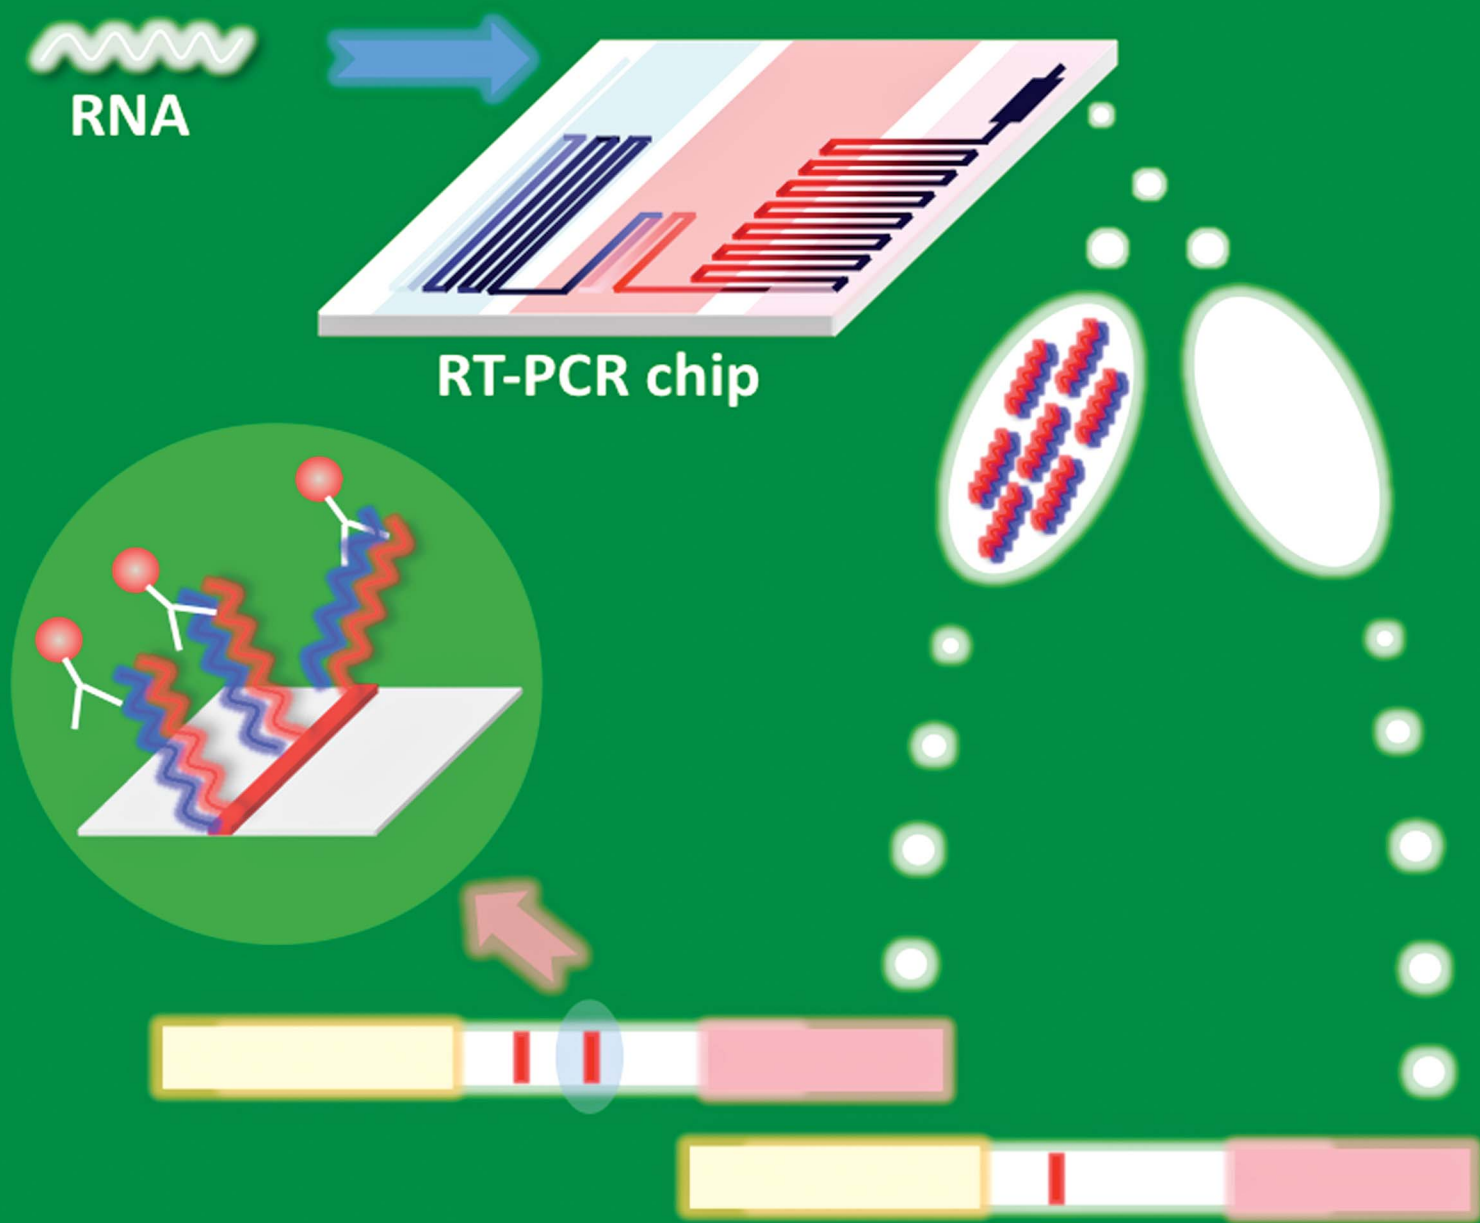

ISSN 0003-2654

RSC Publishing

COMMUNICATION

Naoki Nagatani *et al.*
Detection of influenza virus using a
lateral flow immunoassay for amplified DNA
by a microfluidic RT-PCR chip



0003-2654 (2012) 137:15;1-1